



# Comparison of Restriction Digest Sample on Fragment Analyzer™ (Top) vs. Tapestation (Bottom)

DNF-930  
Qualitative Kit  
5 kV, 60 min

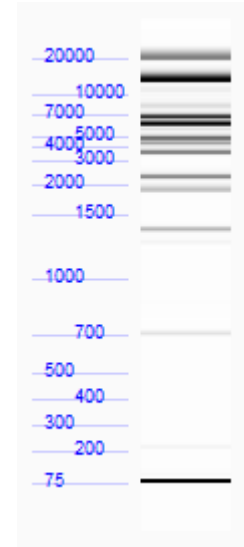

Genomic DNA  
ScreenTape®

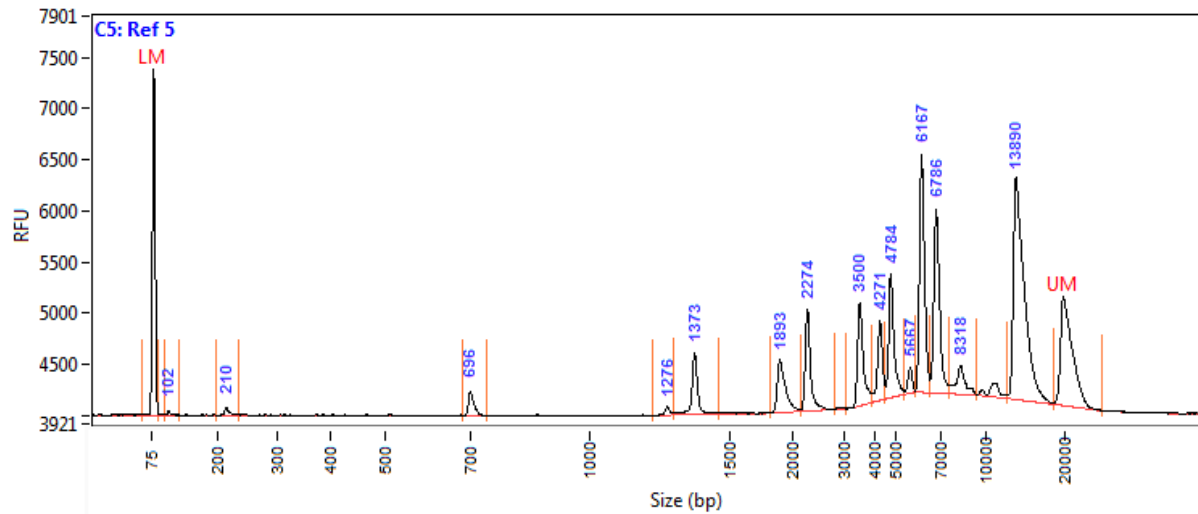