


Loaded two aliquotes of each sample: c.ca 700 ng and 2000 ng

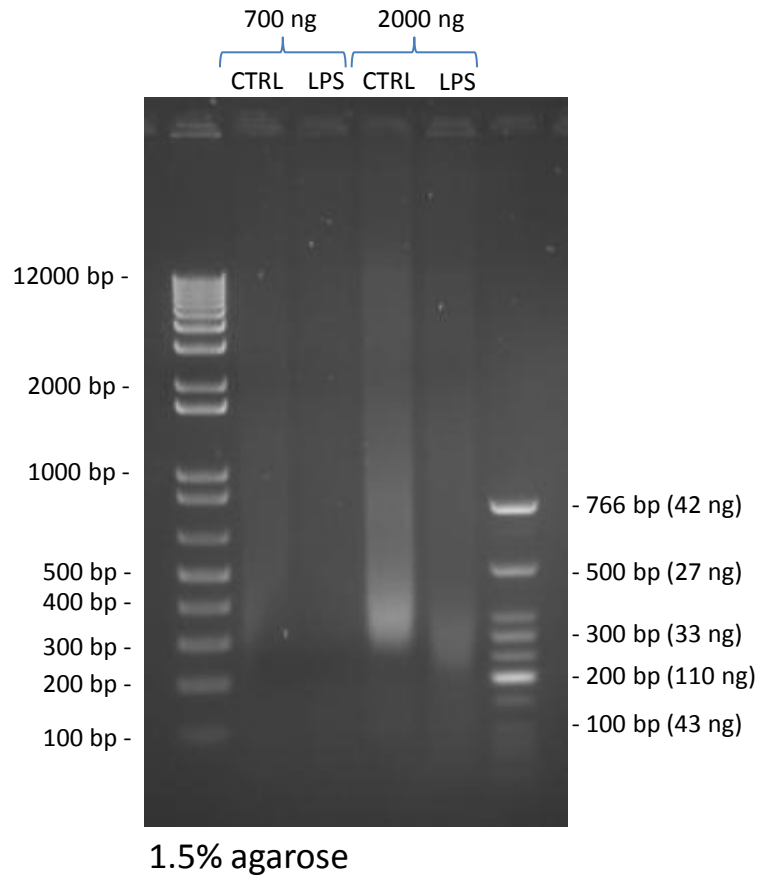

Covaris (Covaris S2) settings:

Duty cycle	10
Intensity	5
Cycles/burst	200
Duration	120 sec