


Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13805695_2014-09-08_16-31-58.xad

Created: 9/8/2014 4:31:57 PM
Modified: 9/8/2014 5:13:23 PM

Electrophoresis File Run Summary

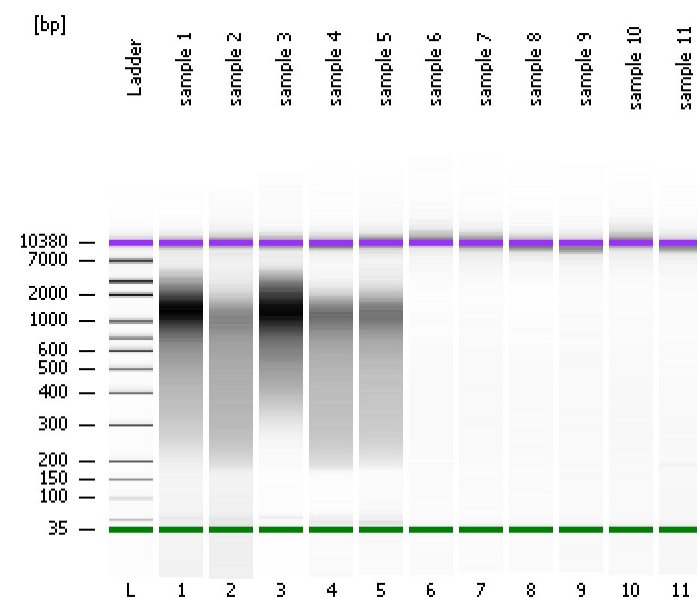

Instrument Information:


Instrument Name: DE13805695 Firmware: C.01.069
Serial#: DE13805695 Type: G2939A

Assay Information:

Assay Origin Path: C:\Program Files\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy
Assay Class: High Sensitivity DNA Assay
Version: 1.03
Assay Comments: Copyright © 2003-2010 Agilent Technologies

Chip Information:

Chip Lot #:
Reagent Kit Lot #:
Chip Comments:

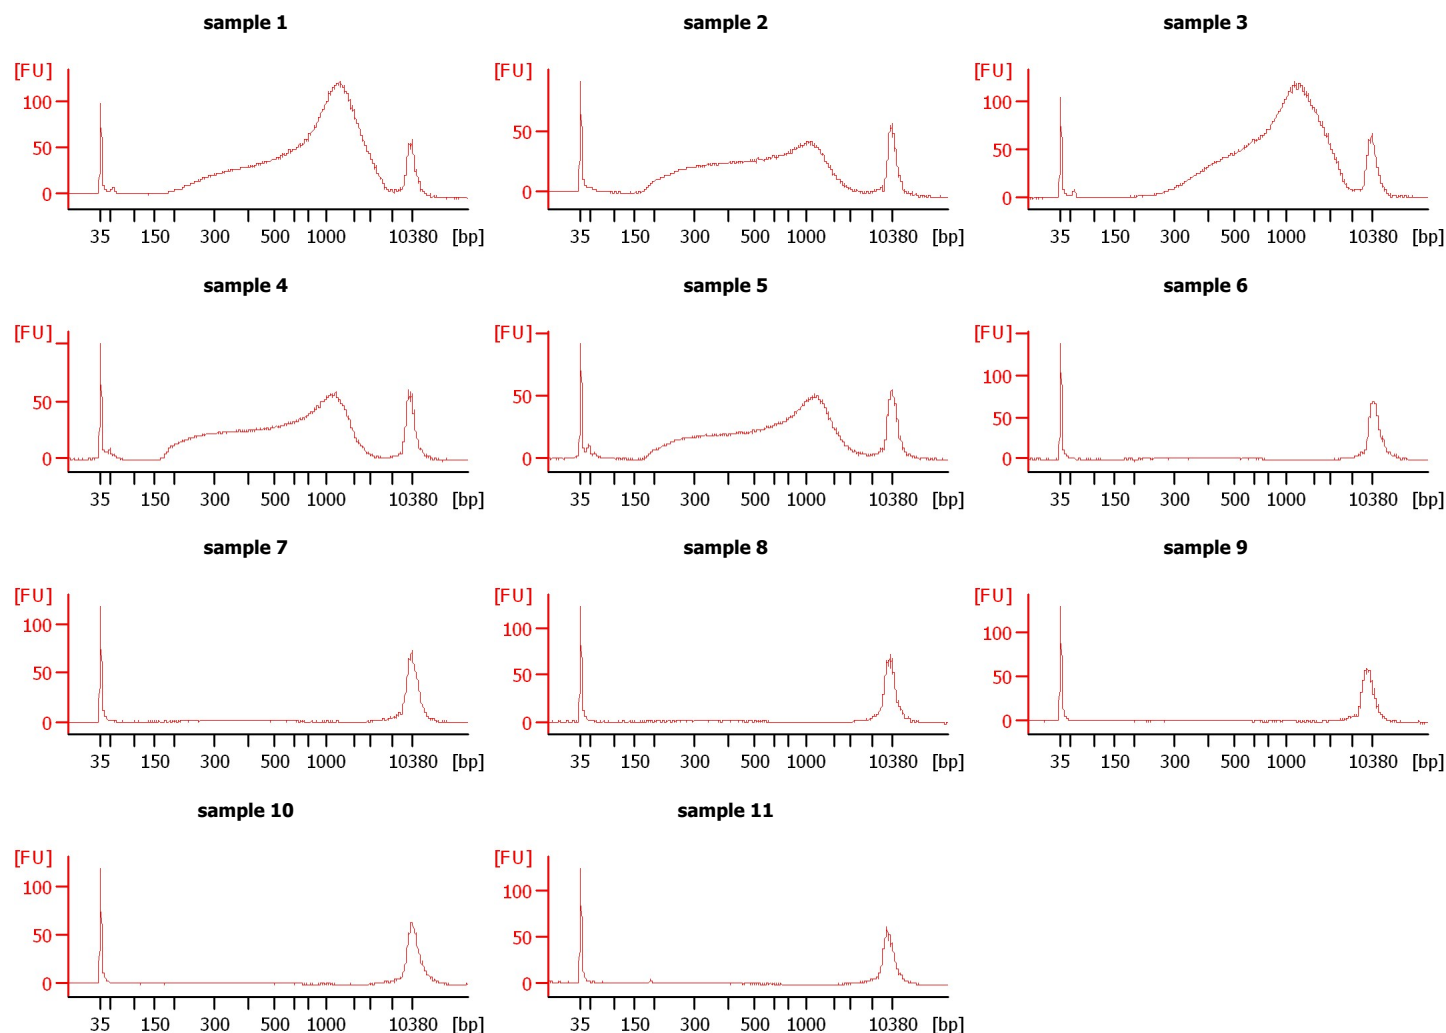

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13805695_2014-09-08_16-31-58.xad

Created: 9/8/2014 4:31:57 PM
Modified: 9/8/2014 5:13:23 PM

Electrophoresis File Run Summary (Chip Summary)

Sample Name	Sample Comment	Rest. Digest	Status	Observation	Result Label	Result Color
sample 1		☐	✓			
sample 2		☐	✓			
sample 3		☐	✓			
sample 4		☐	✓			
sample 5		☐	✓			
sample 6		☐	✓			
sample 7		☐	✓			
sample 8		☐	✓			
sample 9		☐	✓			
sample 10		☐	✓			
sample 11		☐	✓			
Ladder		☐	✓			

Chip Lot #**Reagent Kit Lot #****Chip Comments :**

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13805695_2014-09-08_16-31-58.xad

Created: 9/8/2014 4:31:57 PM
Modified: 9/8/2014 5:13:23 PM

Electrophoresis Assay Details

General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 12
Minimum Visible Range [s] : 32
Maximum Visible Range [s] : 138
Start Analysis Time Range [s] : 33
End Analysis Time Range [s] : 137.5
Ladder Concentration [pg/ μ l] : 1950
Uses Standard Area for Ladder Fragments
Lower Marker Concentration [pg/ μ l] : 125
Upper Marker Concentration [pg/ μ l] : 75
Used Upper Marker for Quantitation
Standard Curve Fit is Point to Point
Show Data Aligned to Lower and Upper Marker

Integrator Settings

Integration Start Time [s] : 33.05
Integration End Time [s] : 137
Slope Threshold : 0.8
Height Threshold [FU] : 5
Area Threshold : 0.1
Width Threshold [s] : 0.6
Baseline Plateau [s] : 0.5

Filter Settings

Filter Width [s] : 0.5
Polynomial Order : 4


Ladder

Ladder Peak	Size	Area
1	35	160
2	50	210
3	100	208
4	150	221
5	200	242
6	300	270
7	400	305
8	500	306
9	600	336
10	700	321
11	1000	366
12	2000	413
13	3000	411
14	7000	400
15	10380	214

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13805695_2014-09-08_16-31-58.xad

Created: 9/8/2014 4:31:57 PM
 Modified: 9/8/2014 5:13:23 PM

Electropherogram Summary

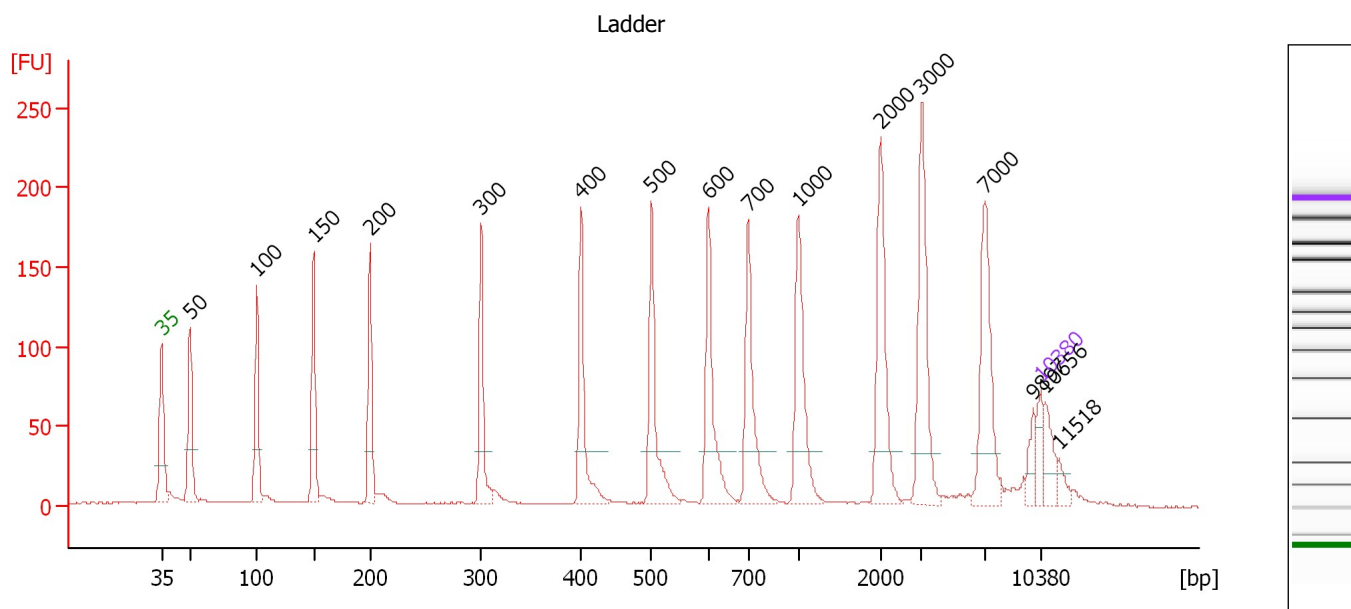

Overall Results for Ladder

Noise: 0.4


Peak table for Ladder

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	50	150.00	4,545.5	Ladder Peak
3	100	150.00	2,272.7	Ladder Peak
4	150	150.00	1,515.2	Ladder Peak
5	200	150.00	1,136.4	Ladder Peak
6	300	150.00	757.6	Ladder Peak
7	400	150.00	568.2	Ladder Peak
8	500	150.00	454.5	Ladder Peak
9	600	150.00	378.8	Ladder Peak
10	700	150.00	324.7	Ladder Peak
11	1,000	150.00	227.3	Ladder Peak
12	2,000	150.00	113.6	Ladder Peak
13	3,000	150.00	75.8	Ladder Peak
14	7,000	150.00	32.5	Ladder Peak
15	9,897	0.00	0.0	
16	10,380	75.00	10.9	Upper Marker
17	10,656	0.00	0.0	
18	11,518	0.00	0.0	

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13805695_2014-09-08_16-31-58.xad

Created: 9/8/2014 4:31:57 PM
 Modified: 9/8/2014 5:13:23 PM

Electropherogram Summary Continued ...

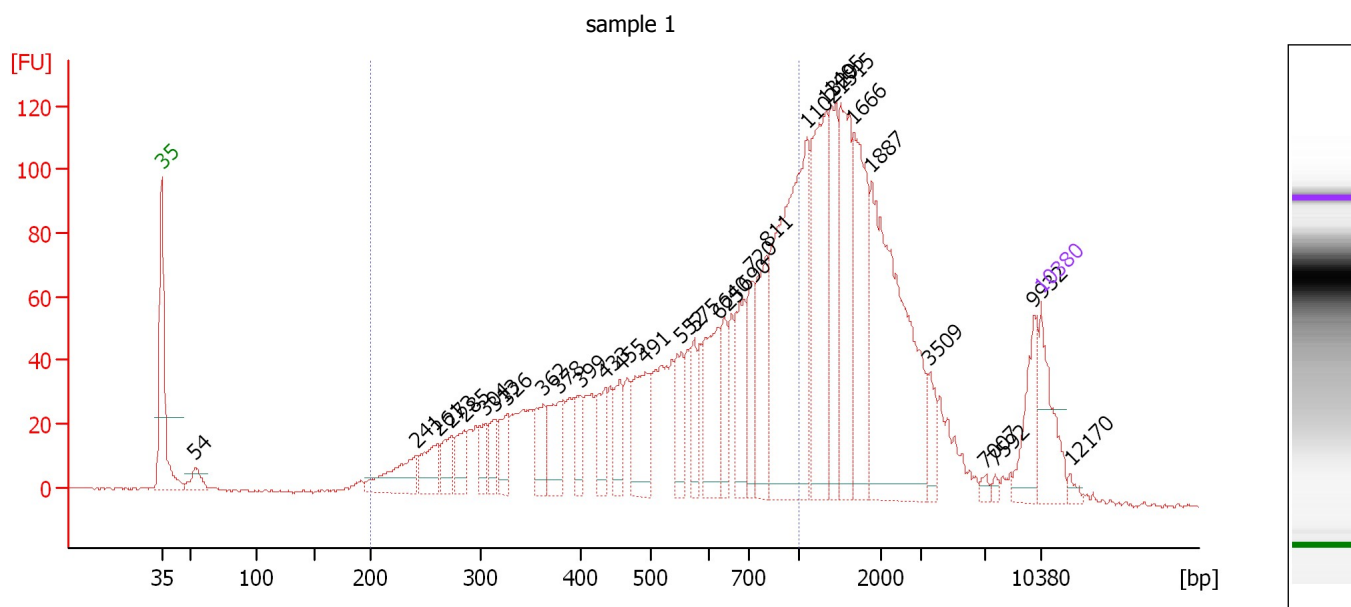

Overall Results for sample 1 : sample 1

Number of peaks found: 32 Corr. Area 1: 1,564.7
 Noise: 0.4

Peak table for sample 1 : sample 1

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	54	35.35	996.3	
3	241	90.54	568.3	
4	261	65.34	379.7	
5	273	49.10	272.6	
6	285	48.84	259.9	
7	304	35.38	176.4	
8	313	44.26	213.9	
9	326	50.75	236.0	
10	362	64.46	269.8	
11	378	73.15	293.4	
12	399	49.18	186.7	
13	433	61.91	216.4	
14	455	55.58	185.0	
15	491	108.26	333.8	
16	552	63.55	174.4	
17	575	47.75	125.8	
18	625	121.16	293.5	
19	640	53.16	125.9	
20	690	94.30	207.0	
21	720	68.39	143.9	
22	811	120.12	224.4	
23	1,102	427.40	587.6	
24	1,329	220.57	251.4	
25	1,405	134.37	144.9	
26	1,515	163.45	163.5	

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13805695_2014-09-08_16-31-58.xad

Created: 9/8/2014 4:31:57 PM
Modified: 9/8/2014 5:13:23 PM

Electropherogram Summary Continued ...**... Peak table for sample 1 : sample 1**


Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
27	1,666	172.96	157.3	
28	1,887	363.36	291.8	
29	3,509	33.35	14.4	
30	7,007	6.97	1.5	
31	7,592	5.10	1.0	
32	9,932	67.36	10.3	
33	10,380	75.00	10.9	Upper Marker
34	12,170	0.00	0.0	

Region table for sample 1 : sample 1

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	1,564.7	56	571	37.2	2,339.61	7,809.2	

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13805695_2014-09-08_16-31-58.xad

Created: 9/8/2014 4:31:57 PM
 Modified: 9/8/2014 5:13:23 PM

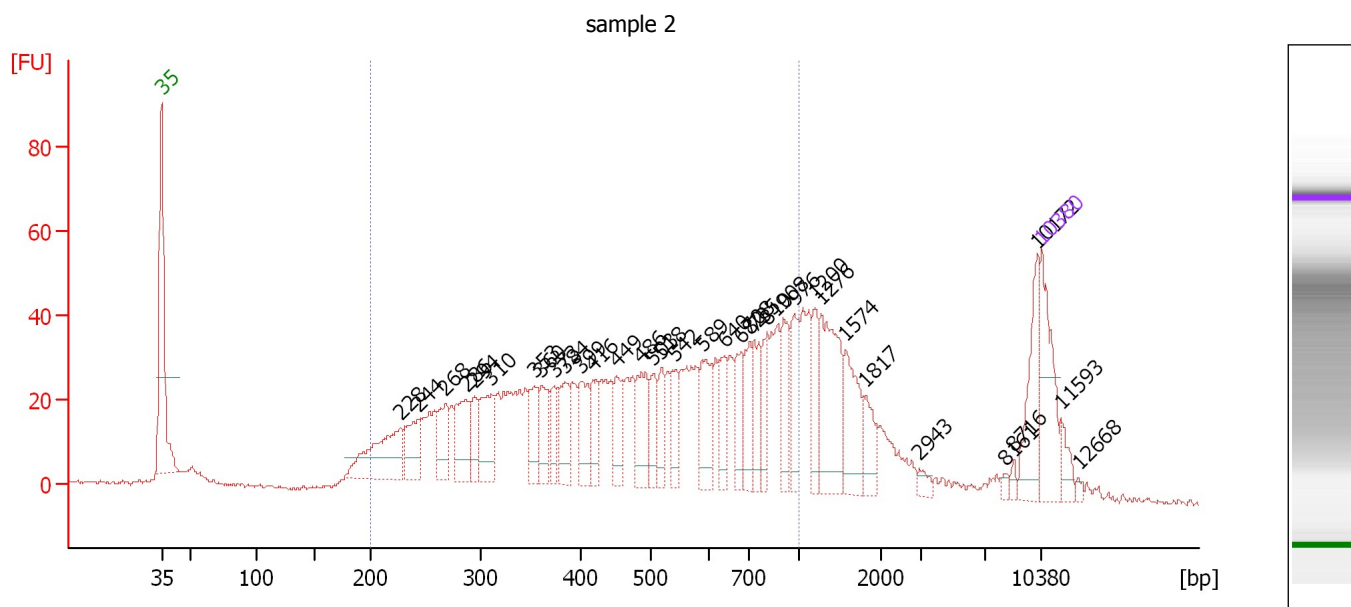Electropherogram Summary Continued ...**Overall Results for sample 2 : sample 2**

Number of peaks found: 35 Corr. Area 1: 1,186.6
 Noise: 0.4

Peak table for sample 2 : sample 2

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	228	115.05	765.8	
3	244	56.66	352.5	
4	268	47.72	270.2	
5	286	66.72	353.3	
6	294	35.73	183.9	
7	310	70.73	345.5	
8	353	43.45	186.6	
9	360	42.83	180.2	
10	373	32.04	130.3	
11	384	49.67	196.0	
12	399	51.38	195.2	
13	416	34.48	125.6	
14	449	39.70	133.9	
15	486	60.12	187.5	
16	503	34.36	103.4	
17	518	35.05	102.6	
18	542	34.35	96.1	
19	589	56.61	145.6	
20	640	35.57	84.3	
21	682	36.73	81.6	
22	708	46.66	99.9	
23	735	38.84	80.1	
24	810	35.79	67.0	
25	908	46.17	77.1	
26	976	45.89	71.3	

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13805695_2014-09-08_16-31-58.xad

Created: 9/8/2014 4:31:57 PM
 Modified: 9/8/2014 5:13:23 PM

Electropherogram Summary Continued ...**... Peak table for sample 2 : sample 2**


Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
27	1,200	36.75	46.4	
28	1,276	105.07	124.8	
29	1,574	61.66	59.4	
30	1,817	29.74	24.8	
31	2,943	8.22	4.2	
32	8,161	4.50	0.8	
33	8,716	5.17	0.9	
34	10,172	56.23	8.4	
35	10,380	75.00	10.9	Upper Marker
36	11,593	0.00	0.0	
37	12,668	0.00	0.0	

Region table for sample 2 : sample 2

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	1,186.6	72	505	40.7	2,012.89	7,706.6	

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13805695_2014-09-08_16-31-58.xad

Created: 9/8/2014 4:31:57 PM
 Modified: 9/8/2014 5:13:23 PM

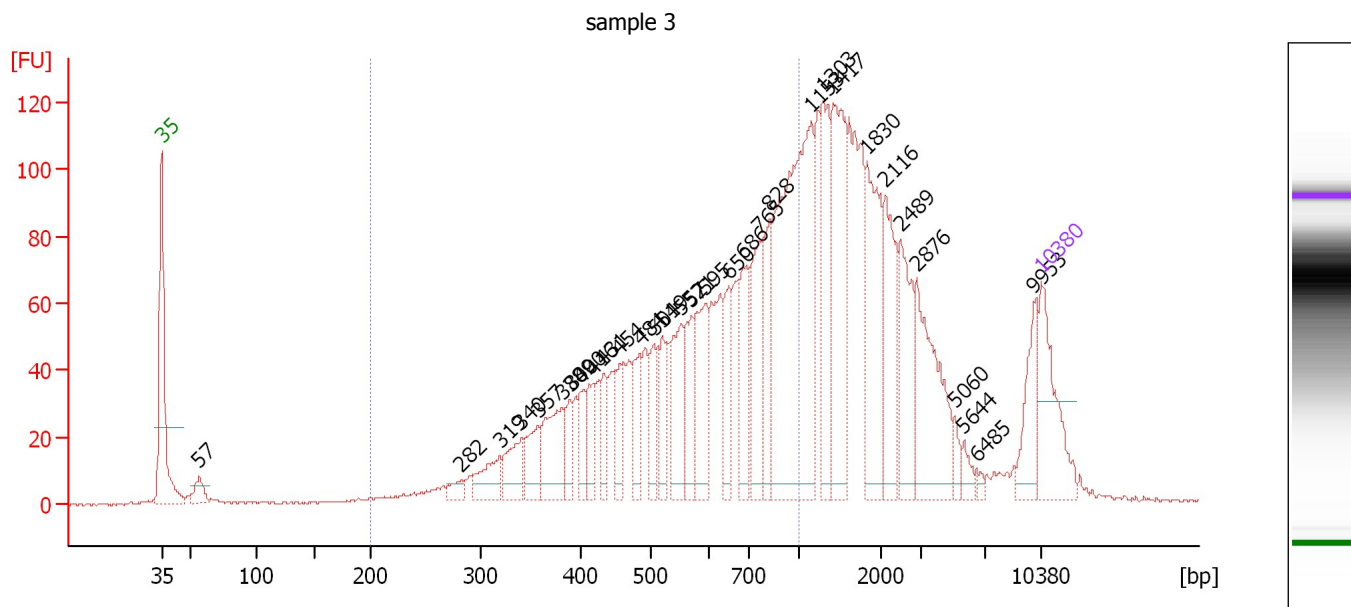Electropherogram Summary Continued ...**Overall Results for sample 3 : sample 3**

Number of peaks found: 32 Corr. Area 1: 1,457.9
 Noise: 0.4

Peak table for sample 3 : sample 3

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	57	24.27	647.4	
3	282	15.26	82.0	
4	319	42.99	204.5	
5	340	46.27	206.1	
6	357	43.05	182.7	
7	380	77.70	309.5	
8	389	27.72	108.1	
9	400	30.12	114.2	
10	416	38.46	140.0	
11	431	33.38	117.3	
12	454	35.60	118.7	
13	484	42.69	133.8	
14	504	41.72	125.3	
15	519	42.53	124.2	
16	552	73.65	202.2	
17	571	51.11	135.7	
18	595	85.20	216.8	
19	650	50.18	116.9	
20	686	71.32	157.4	
21	765	86.83	172.0	
22	828	65.07	119.1	
23	1,153	338.42	444.7	
24	1,303	96.13	111.8	
25	1,417	140.01	149.7	
26	1,830	112.68	93.3	

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13805695_2014-09-08_16-31-58.xad

Created: 9/8/2014 4:31:57 PM
Modified: 9/8/2014 5:13:23 PM

Electropherogram Summary Continued ...**... Peak table for sample 3 : sample 3**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
27	2,116	86.85	62.2	
28	2,489	74.95	45.6	
29	2,876	115.55	60.9	
30	5,060	11.44	3.4	
31	5,644	11.90	3.2	
32	6,485	4.25	1.0	
33	9,953	48.87	7.4	
34	10,380	75.00	10.9	Upper Marker


Region table for sample 3 : sample 3

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	1,457.9	54	603	32.1	1,614.54	4,767.3	

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13805695_2014-09-08_16-31-58.xad

Created: 9/8/2014 4:31:57 PM
 Modified: 9/8/2014 5:13:23 PM

Electropherogram Summary Continued ...

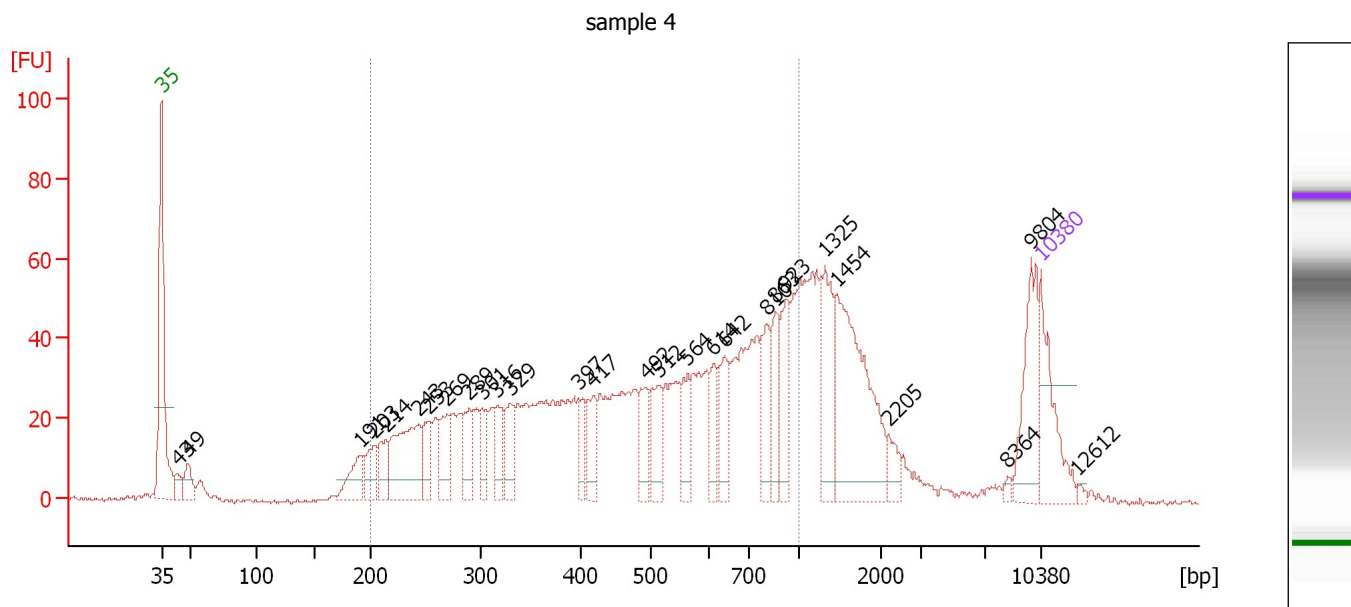

Overall Results for sample 4 : sample 4

Number of peaks found: 28 Corr. Area 1: 1,225.6
 Noise: 0.5

Peak table for sample 4 : sample 4

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	43	22.29	777.2	
3	49	33.16	1,023.4	
4	191	51.99	412.8	
5	203	43.57	325.4	
6	214	43.84	310.3	
7	243	142.61	887.8	
8	253	44.89	268.9	
9	269	52.16	293.3	
10	289	50.11	262.6	
11	301	38.07	191.7	
12	316	43.58	208.8	
13	329	45.81	210.8	
14	397	33.85	129.2	
15	417	46.35	168.5	
16	492	48.19	148.5	
17	512	58.26	172.5	
18	564	42.34	113.8	
19	614	35.87	88.5	
20	642	57.52	135.8	
21	810	56.52	105.7	
22	863	51.65	90.7	
23	923	60.37	99.1	
24	1,325	79.08	90.5	
25	1,454	205.90	214.5	
26	2,205	19.18	13.2	

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13805695_2014-09-08_16-31-58.xad

Created: 9/8/2014 4:31:57 PM
Modified: 9/8/2014 5:13:23 PM

Electropherogram Summary Continued ...**... Peak table for sample 4 : sample 4**


Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
27	8,364	4.39	0.8	
28	9,804	80.05	12.4	
29	10,380	75.00	10.9	Upper Marker
30	12,612	0.00	0.0	

Region table for sample 4 : sample 4

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	1,225.6	70	514	41.5	2,030.73	7,771.4	

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13805695_2014-09-08_16-31-58.xad

Created: 9/8/2014 4:31:57 PM
 Modified: 9/8/2014 5:13:23 PM

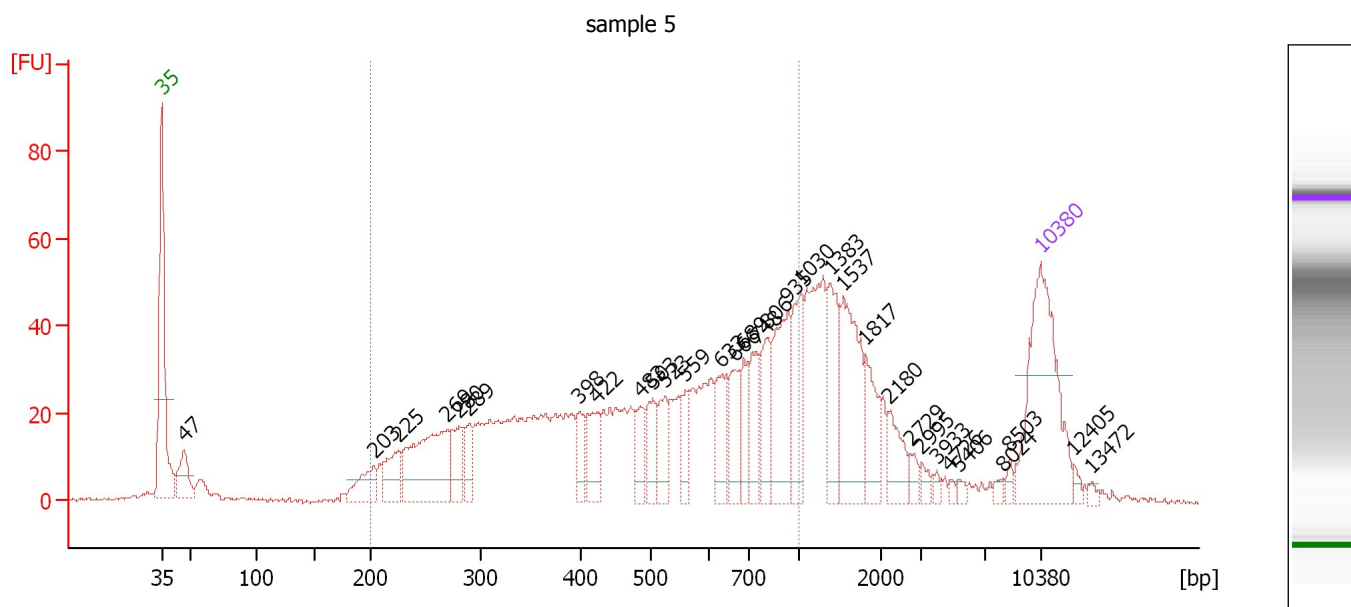Electropherogram Summary Continued ...**Overall Results for sample 5 : sample 5**

Number of peaks found: 32 Corr. Area 1: 973.8
 Noise: 0.4

Peak table for sample 5 : sample 5

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	47	28.20	905.8	
3	203	22.89	170.5	
4	225	23.99	161.4	
5	269	79.56	447.6	
6	280	24.39	131.9	
7	289	16.66	87.2	
8	398	15.05	57.3	
9	422	24.29	87.2	
10	483	17.13	53.7	
11	503	21.01	63.3	
12	523	19.92	57.7	
13	559	14.70	39.8	
14	633	24.33	58.2	
15	666	24.25	55.2	
16	689	17.55	38.6	
17	748	26.43	53.5	
18	806	27.66	52.0	
19	935	48.51	78.6	
20	1,030	32.78	48.2	
21	1,383	35.27	38.6	
22	1,537	54.54	53.8	
23	1,817	22.62	18.9	
24	2,180	17.03	11.8	
25	2,729	5.28	2.9	
26	2,995	4.34	2.2	

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13805695_2014-09-08_16-31-58.xad

Created: 9/8/2014 4:31:57 PM
Modified: 9/8/2014 5:13:23 PM

Electropherogram Summary Continued ...**... Peak table for sample 5 : sample 5**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
27	3,933	2.79	1.1	
28	4,726	1.97	0.6	
29	5,406	2.54	0.7	
30	8,024	2.77	0.5	
31	8,503	3.27	0.6	
32	10,380	75.00	10.9	Upper Marker
33	12,405	0.00	0.0	
34	13,472	0.00	0.0	


Region table for sample 5 : sample 5

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	973.8	67	523	40.9	812.11	3,036.0	

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13805695_2014-09-08_16-31-58.xad

Created: 9/8/2014 4:31:57 PM
 Modified: 9/8/2014 5:13:23 PM

Electropherogram Summary Continued ...

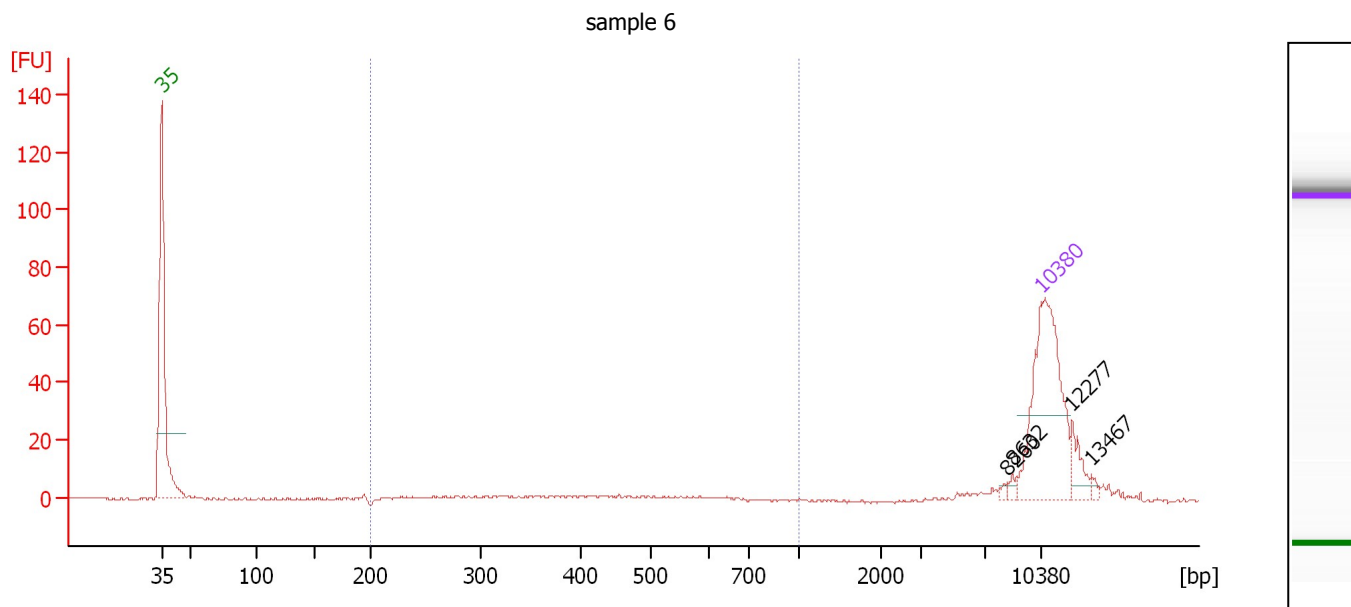

Overall Results for sample 6 : sample 6

Number of peaks found: 4 Corr. Area 1: 14.8
 Noise: 0.4

Peak table for sample 6 : sample 6


Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	8,260	1.54	0.3	
3	8,632	2.16	0.4	
4	10,380	75.00	10.9	Upper Marker
5	12,277	0.00	0.0	
6	13,467	0.00	0.0	

Region table for sample 6 : sample 6

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	14.8	24	403	24.3	10.03	41.1	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13805695_2014-09-08_16-31-58.xad

Created: 9/8/2014 4:31:57 PM
 Modified: 9/8/2014 5:13:23 PM

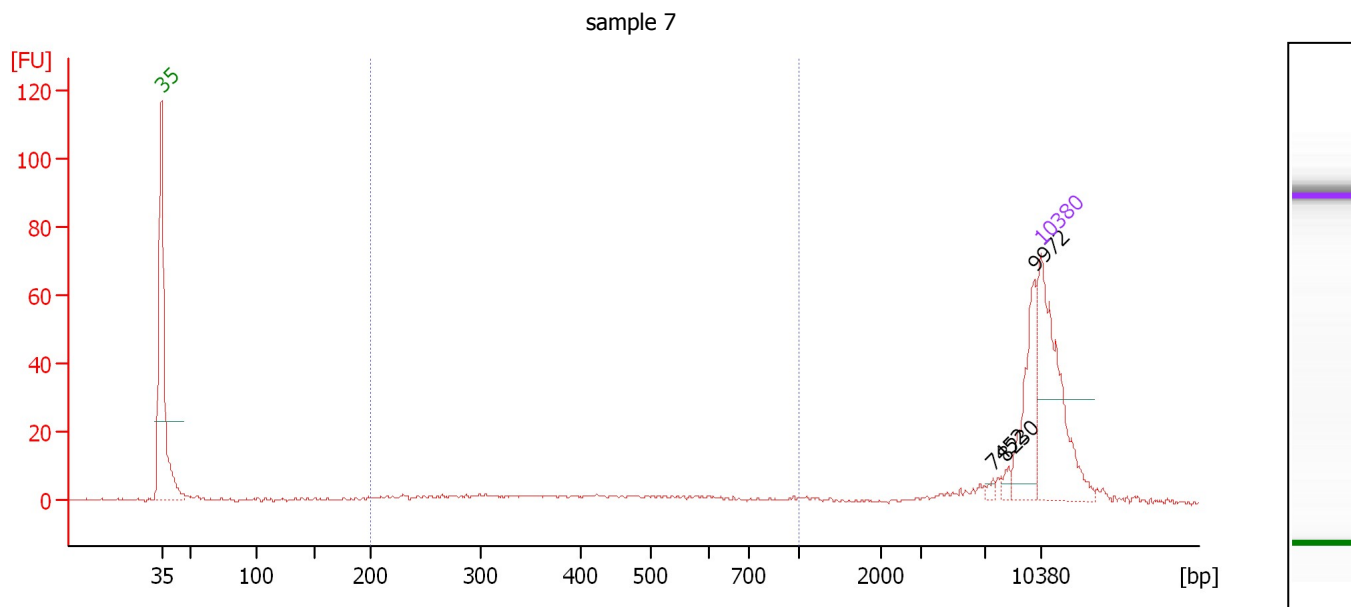Electropherogram Summary Continued ...**Overall Results for sample 7 : sample 7**

Number of peaks found: 3 Corr. Area 1: 52.4
 Noise: 0.4

Peak table for sample 7 : sample 7

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	7,452	2.39	0.5	
3	8,230	3.11	0.6	
4	9,972	38.87	5.9	
5	10,380	75.00	10.9	Upper Marker


Region table for sample 7 : sample 7

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	52.4	32	428	38.9	45.71	195.7	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13805695_2014-09-08_16-31-58.xad

Created: 9/8/2014 4:31:57 PM
 Modified: 9/8/2014 5:13:23 PM

Electropherogram Summary Continued ...

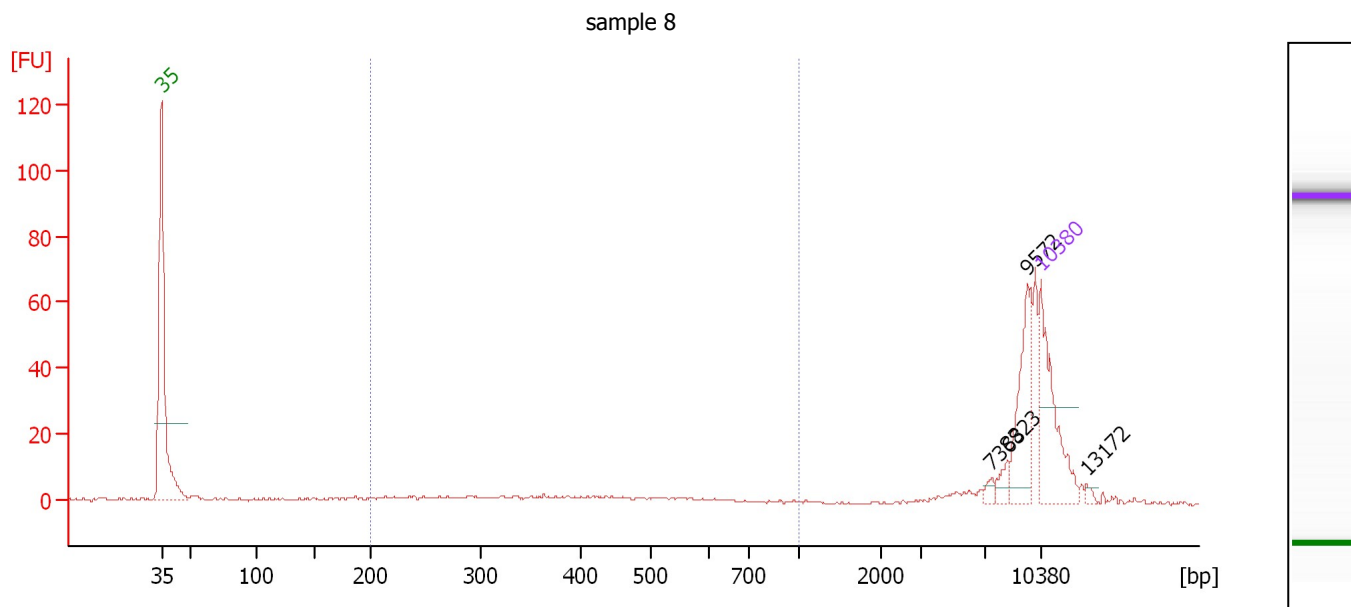

Overall Results for sample 8 : sample 8

Number of peaks found: 4 Corr. Area 1: 31.2
 Noise: 0.4

Peak table for sample 8 : sample 8


Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	7,368	5.72	1.2	
3	8,323	9.89	1.8	
4	9,572	63.65	10.1	
5	10,380	75.00	10.9	Upper Marker
6	13,172	0.00	0.0	

Region table for sample 8 : sample 8

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	31.2	19	388	30.3	43.27	192.4	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13805695_2014-09-08_16-31-58.xad

Created: 9/8/2014 4:31:57 PM
 Modified: 9/8/2014 5:13:23 PM

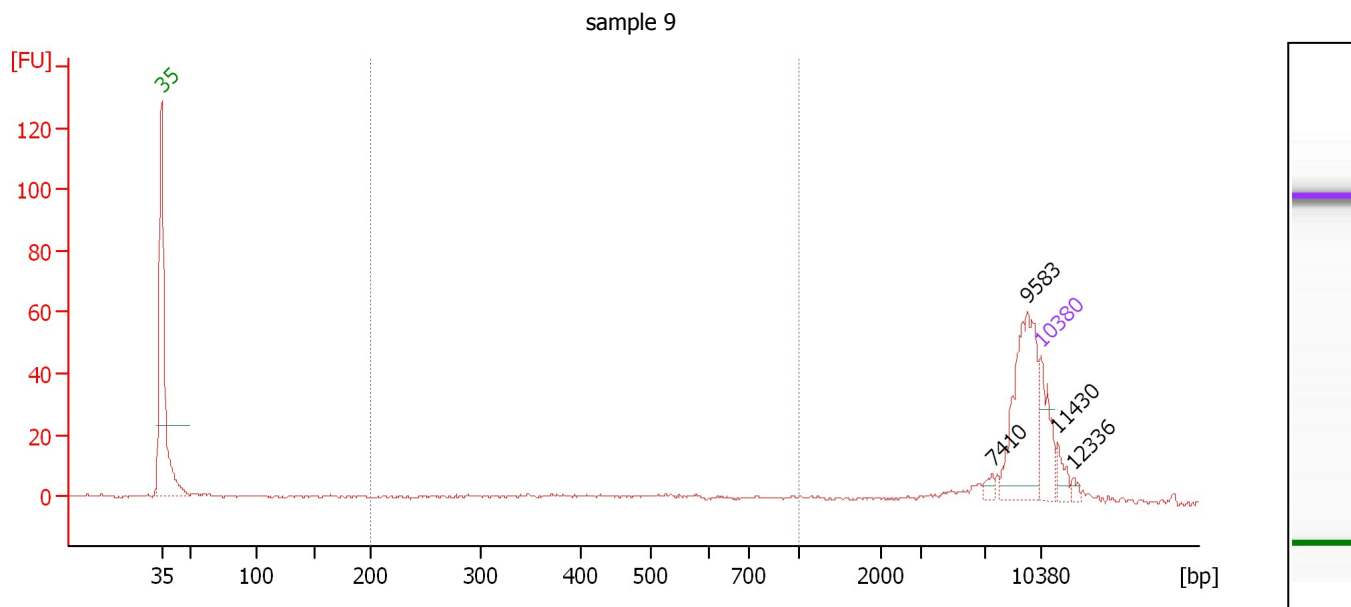Electropherogram Summary Continued ...**Overall Results for sample 9 : sample 9**

Number of peaks found: 4 Corr. Area 1: 50.2
 Noise: 0.5

Peak table for sample 9 : sample 9

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	7,410	13.23	2.7	
3	9,583	227.81	36.0	
4	10,380	75.00	10.9	Upper Marker
5	11,430	0.00	0.0	
6	12,336	0.00	0.0	


Region table for sample 9 : sample 9

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	50.2	19	475	39.2	138.38	543.0	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13805695_2014-09-08_16-31-58.xad

Created: 9/8/2014 4:31:57 PM
 Modified: 9/8/2014 5:13:23 PM

Electropherogram Summary Continued ...

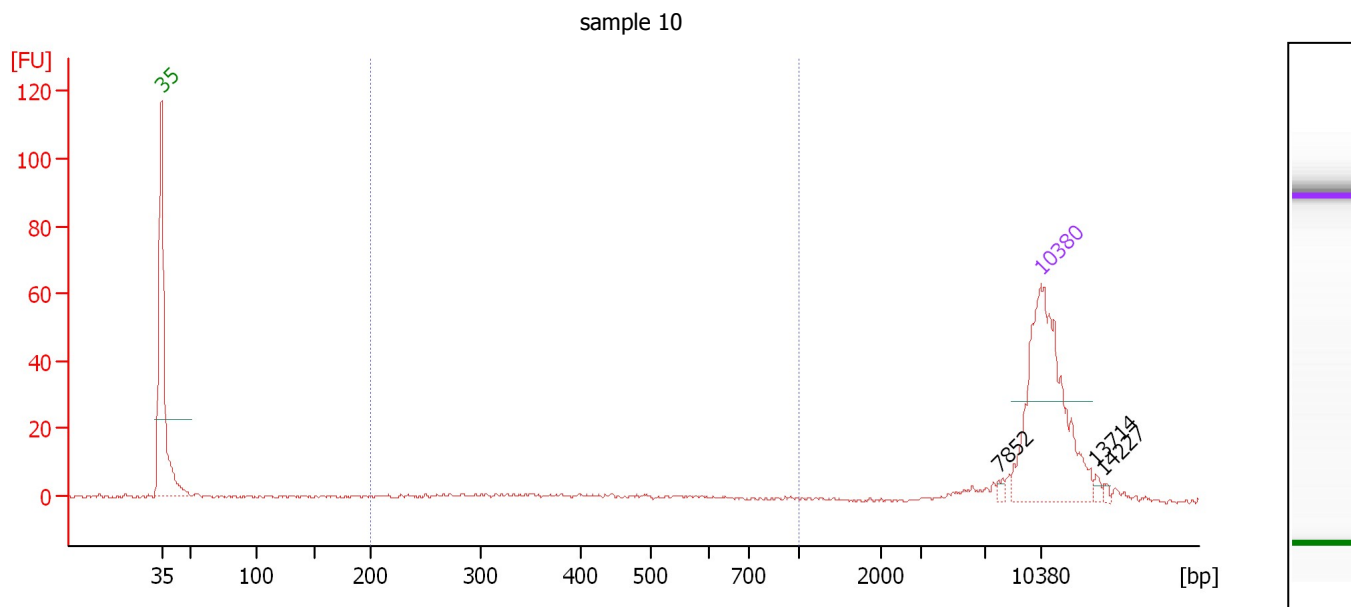

Overall Results for sample 10 : sample 10

Number of peaks found: 3 Corr. Area 1: 44.4
 Noise: 0.5

Peak table for sample 10 : sample 10

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	7,852	1.66	0.3	
3	10,380	75.00	10.9	Upper Marker
4	13,714	0.00	0.0	
5	14,227	0.00	0.0	


Region table for sample 10 : sample 10

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	44.4	46	441	39.4	26.17	109.1	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13805695_2014-09-08_16-31-58.xad

Created: 9/8/2014 4:31:57 PM
 Modified: 9/8/2014 5:13:23 PM

Electropherogram Summary Continued ...

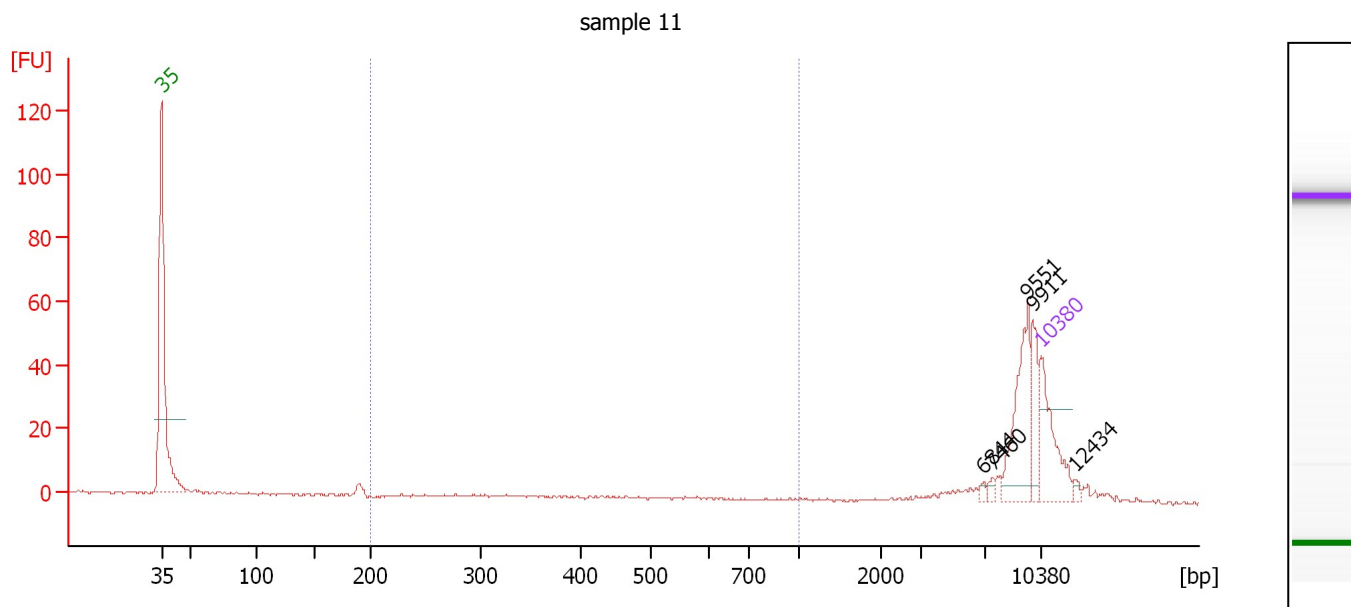

Overall Results for sample 11 : sample 11

Number of peaks found: 5 Corr. Area 1: 8.3
 Noise: 0.4

Peak table for sample 11 : sample 11


Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	6,844	4.98	1.1	
3	7,460	6.54	1.3	
4	9,551	108.77	17.3	
5	9,911	45.04	6.9	
6	10,380	75.00	10.9	Upper Marker
7	12,434	0.00	0.0	

Region table for sample 11 : sample 11

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	8.3	5	439	37.8	17.58	71.7	Blue

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13805695_2014-09-08_16-31-58.xad

Created: 9/8/2014 4:31:57 PM
Modified: 9/8/2014 5:13:23 PM

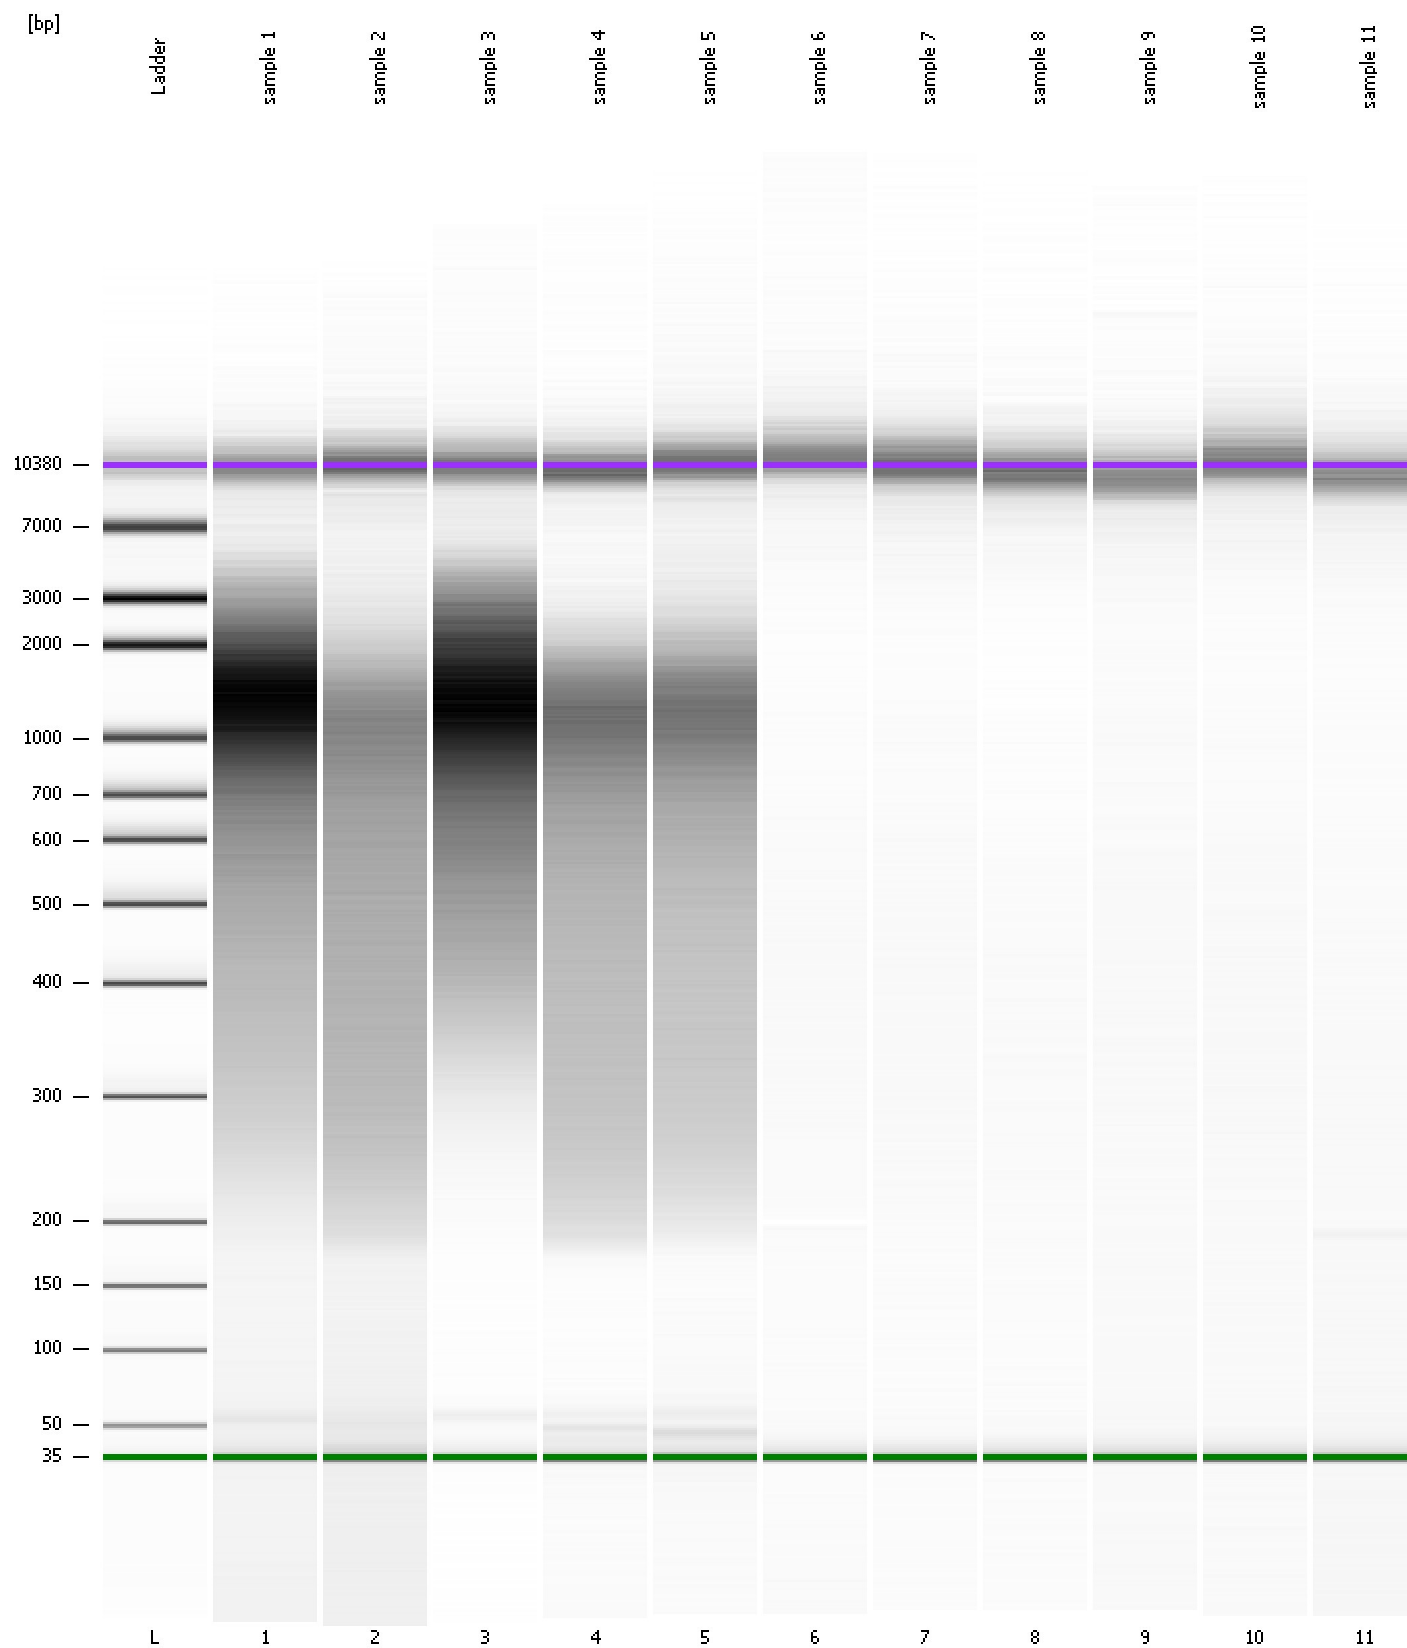
Gel Image

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13805695_2014-09-08_16-31-58.xad

Created: 9/8/2014 4:31:57 PM
Modified: 9/8/2014 5:13:23 PM

Curves

Standard Curve

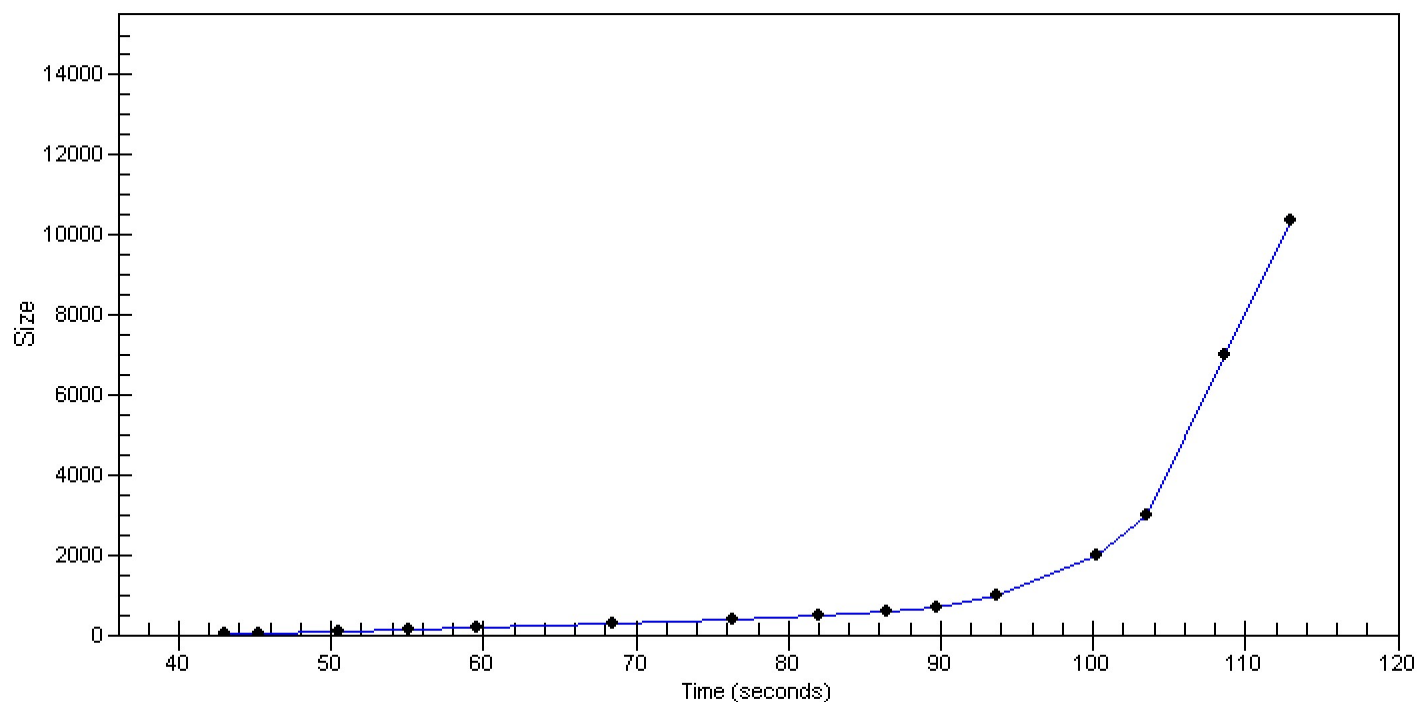

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13805695_2014-09-08_16-31-58.xad

Created: 9/8/2014 4:31:57 PM
 Modified: 9/8/2014 5:13:23 PM

Run Logbook

Description	Number	Source	Category	Sub Category	Time	Time Zone	User	Host
Run ended on port 4 (Number of wells acquired: 12)		Instrument	Run		9/8/2014 5:13:19 PM	(GMT +05:30) India Standard Time	Dr KV Bhutt	DR-EF97DAB0143D
Run started on port 4 (File: C:\Program Files\Agilent\2100 bioanalyzer\2100 expert\Data\2014-09-08\2100 expert_High Sensitivity DNA Assay_DE13805695_2014-09-08_16-31-58.xad)		Instrument	Run		9/8/2014 4:32:04 PM	(GMT +05:30) India Standard Time	Dr KV Bhutt	DR-EF97DAB0143D
Product Number : G2939A		Instrument	Run		9/8/2014 4:32:04 PM	(GMT +05:30) India Standard Time	Dr KV Bhutt	DR-EF97DAB0143D
Name :		Instrument	Run		9/8/2014 4:32:04 PM	(GMT +05:30) India Standard Time	Dr KV Bhutt	DR-EF97DAB0143D
Vendor : Agilent Technologies		Instrument	Run		9/8/2014 4:32:04 PM	(GMT +05:30) India Standard Time	Dr KV Bhutt	DR-EF97DAB0143D
Serial# : DE13805695		Instrument	Run		9/8/2014 4:32:04 PM	(GMT +05:30) India Standard Time	Dr KV Bhutt	DR-EF97DAB0143D
Firmware : C.01.069		Instrument	Run		9/8/2014 4:32:04 PM	(GMT +05:30) India Standard Time	Dr KV Bhutt	DR-EF97DAB0143D
Cartridge : Electrode		Instrument	Run		9/8/2014 4:32:04 PM	(GMT +05:30) India Standard Time	Dr KV Bhutt	DR-EF97DAB0143D